


MASS SPECTROMETRY REPORT

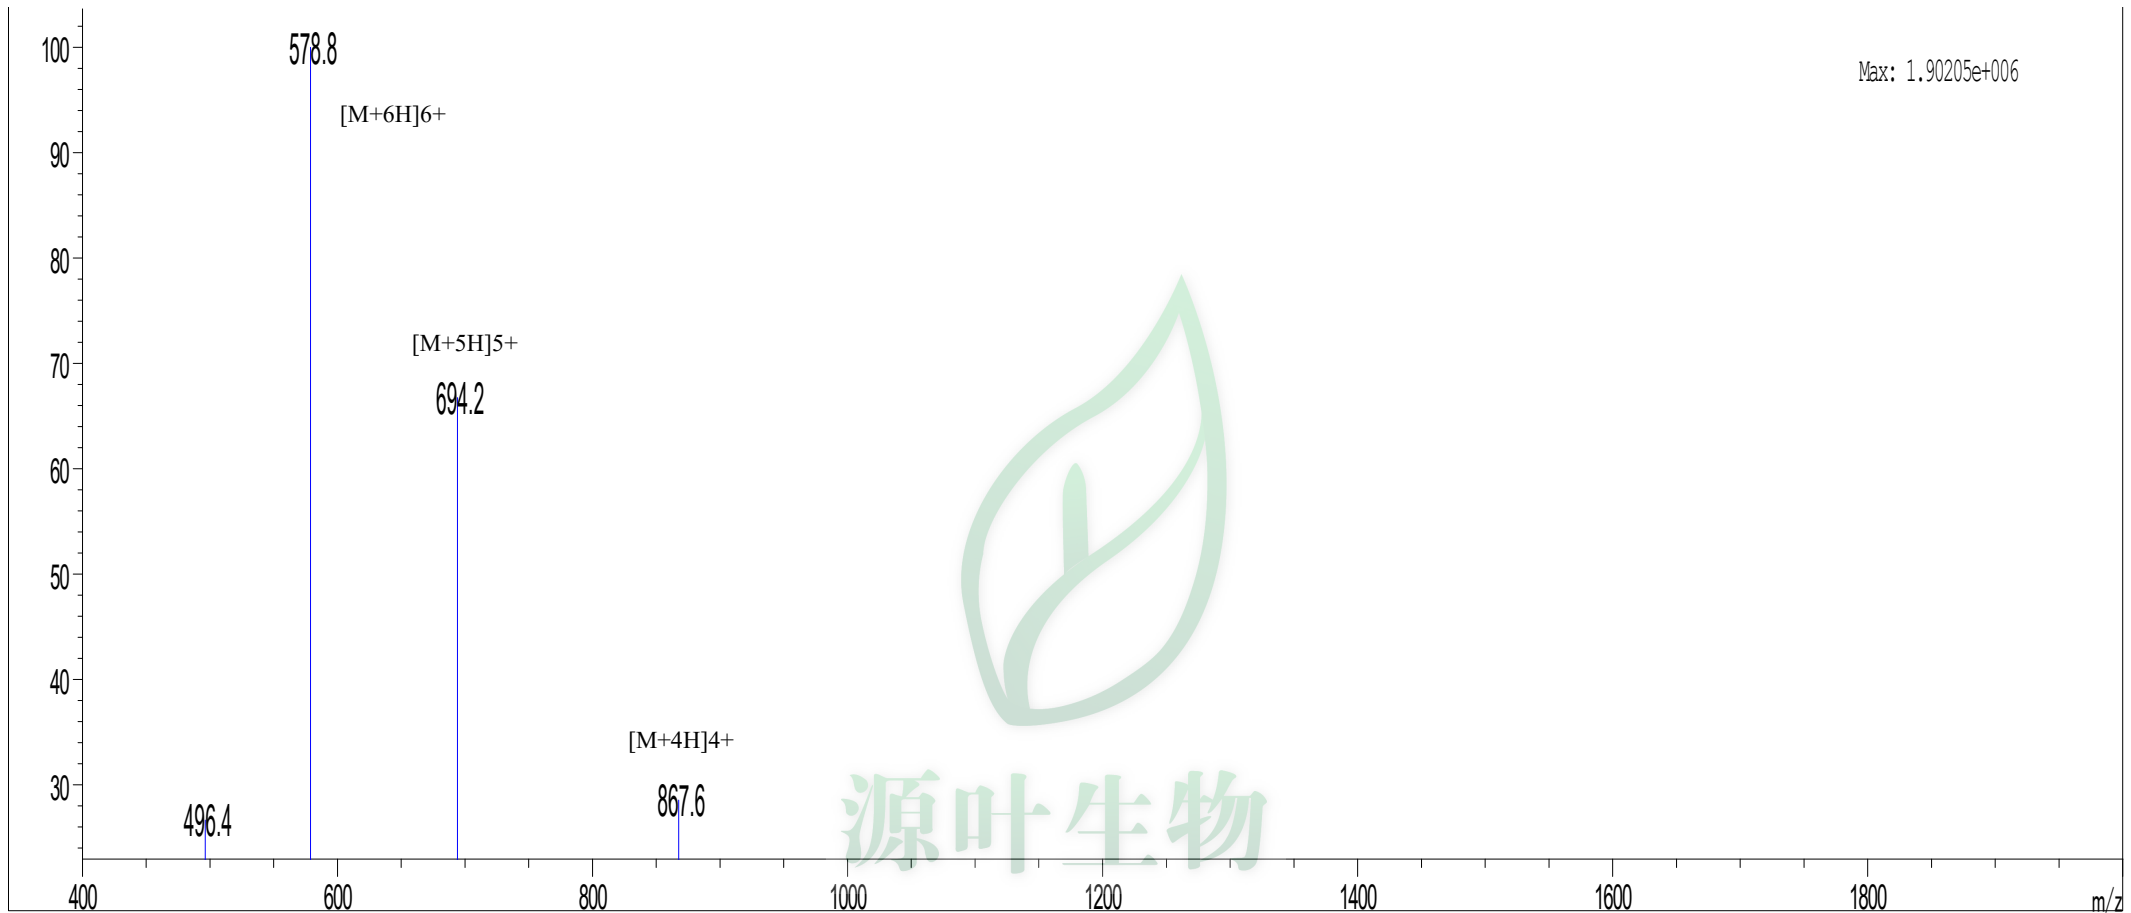

Sample Description

Analyzed date: 2020-06-17
Analyst: YU
Sample: β -内啡肽, 鼠 YQ-31
M.W.: 3466.41
Lot. No.: P200608-CL402074

Instrument

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

Agilent-6125B

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50%ACN