


Sample Name	S25092	Position	P1-A4	Instrument Name	Instrument 1
User Name		Inj Vol	5	InjPosition	
Sample Type	Sample	IRM Calibration Status	Success	Data Filename	S25092
ACQ Method	MS-191123.m	Comment		Acquired Time	1/19/2020 11:41:48 AM



Sample Name	S25092	Position	P1-A4	Instrument Name	Instrument 1
User Name		Inj Vol	5	InjPosition	
Sample Type	Sample	IRM Calibration Status	Success	Data Filename	S25092
ACQ Method	MS-191123.m	Comment		Acquired Time	1/19/2020 11:21:55 AM

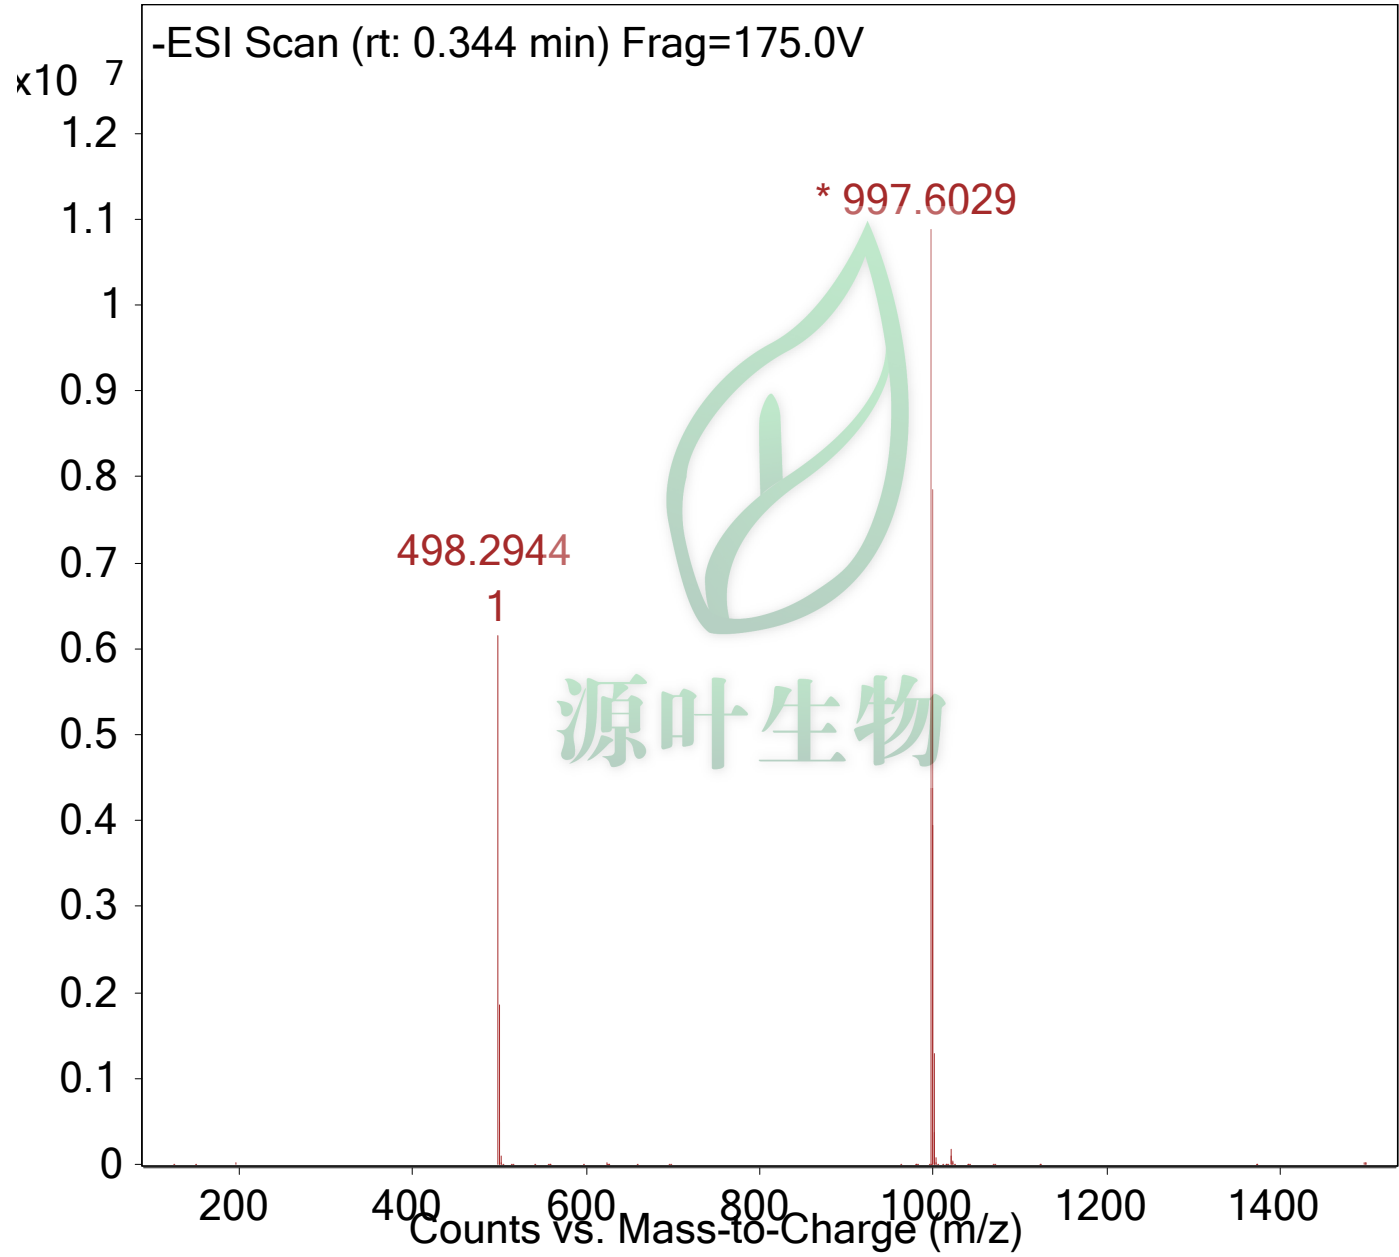