


7.309
7.283
6.257
6.254
6.232
6.229
5.913
5.261
5.238
5.232
4.165
4.155
4.145
3.319
2.781
2.768
2.753
2.738
2.724
2.608
2.602
2.574
2.543
2.527
2.502
2.468
2.454
2.421
2.410
2.189
2.154
2.083
2.058

NAME S65472
EXPNO 4000
PROCNO 1
Date_ 20200403
Time_ 18.29 h
INSTRUM Avance
PROBHD 5 mm
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 8
DS 0
SWH 8620.689 Hz
FIDRES 0.263083 Hz
AQ 3.8011379 sec
RG 100
DW 58.000 usec
DE 12.49 usec
TE 300.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.1819009 MHz
NUC1 1H
P1 9.56 usec
SI 65536
SF 400.1800019 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

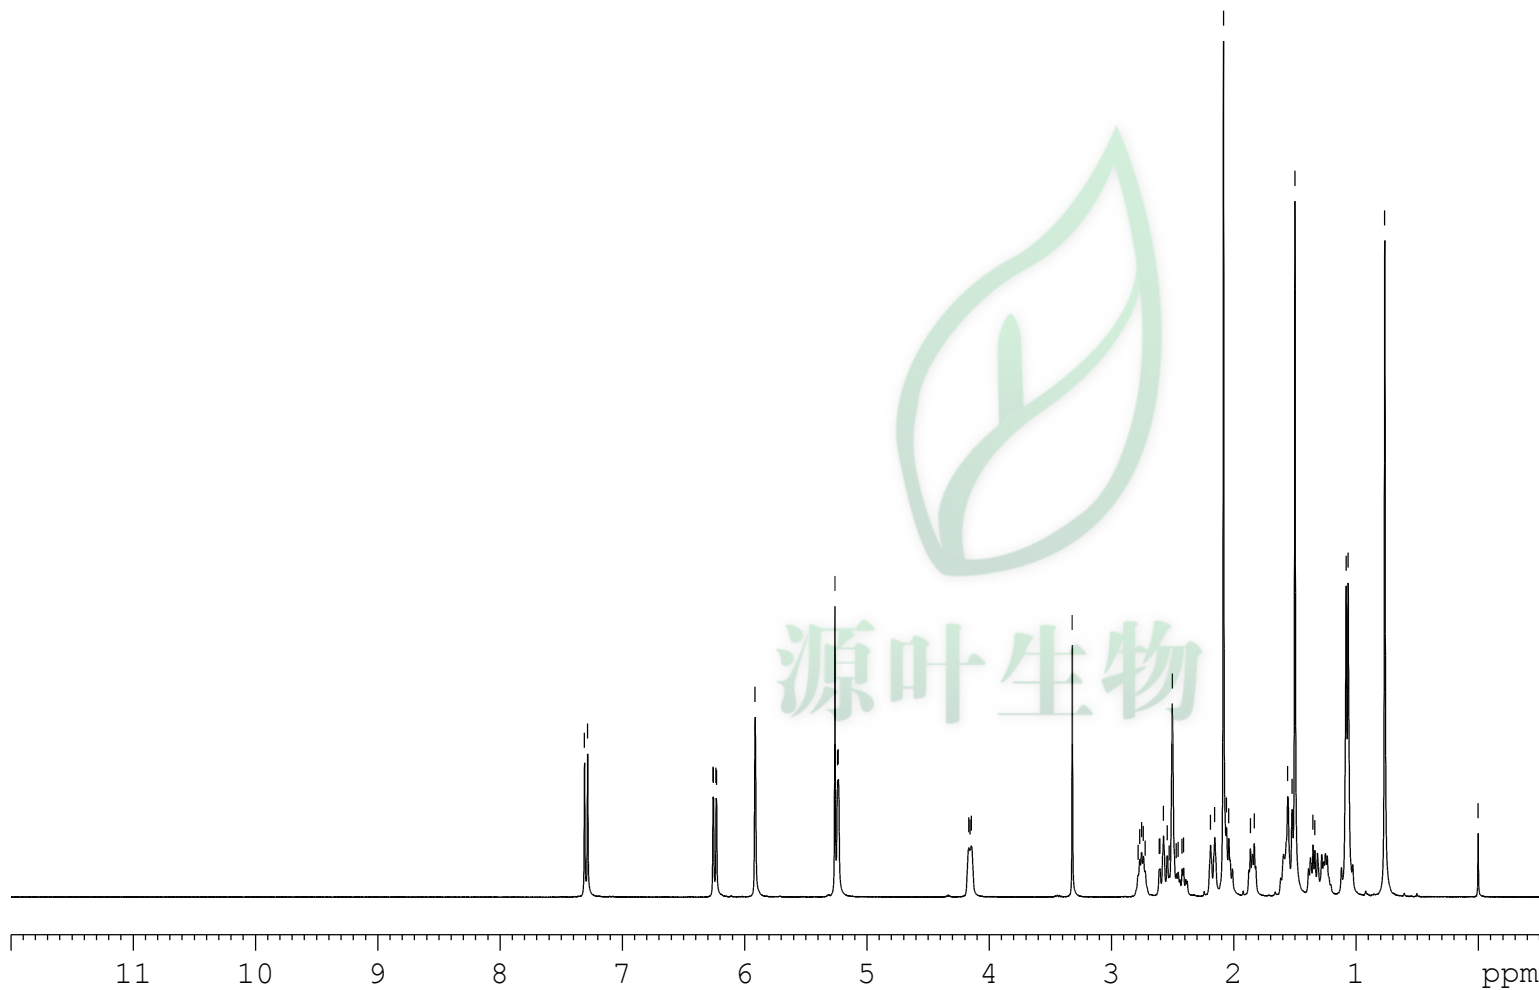

1.00
0.98
1.00
2.03
1.00
0.76
1.01
1.03
0.77
1.03
4.04
1.07
5.00
2.28
4.08
3.07