


Date Acquired: 2019/5/28 14:59:17
Tray# : 1
Vial#: 3
Injection Volume: 1
Processed by: Admin

Peak#:1 Ret.Time:Averaged 7.000-7.017(Scan#:841-843)
BG Mode:Calc 6.850<->7.208(823<->866)
Mass Peaks:3 Base Peak:752.95(360486) Polarity:Neg Segment1 - Event1

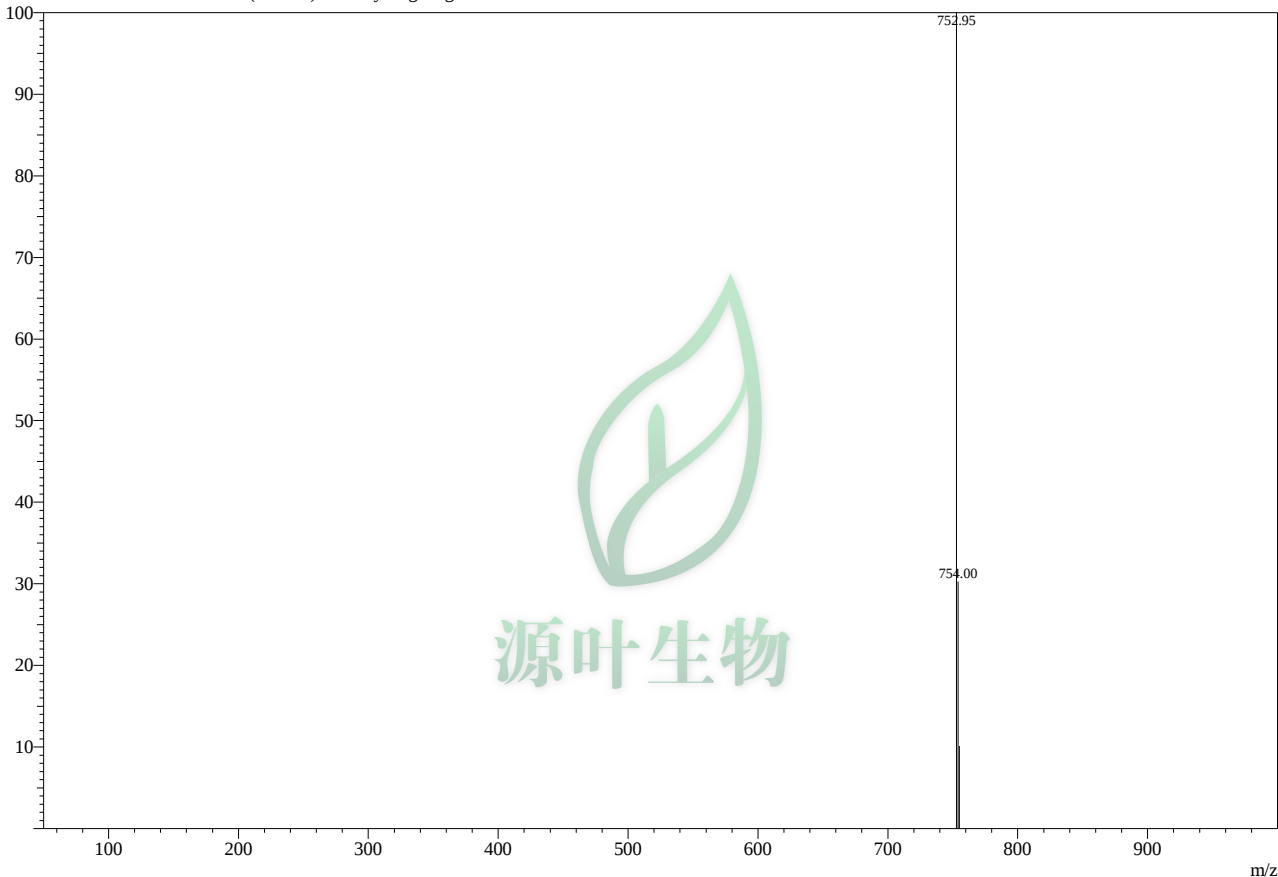

Peak#:1 Ret.Time:
BG Mode:Calc 6.850<->7.208(823<->866)
Mass Peaks:3 Base Peak:752.95(360486) Polarity:Neg Segment1 - Event1

#	m/z	Abs.Inten.	Rel.Inten.	Charge	Polarity	Monoisotopic
1	752.95	360486	100.0			
2	754.00	109134	30.27			