
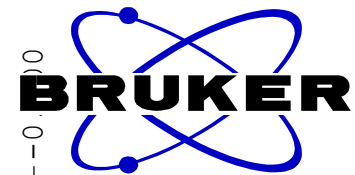


8.716
8.701
8.691
8.681
8.681
8.681
8.061
8.061
8.041
8.041
7.761
7.751
7.741
7.721
7.531
7.511
7.511
7.491
6.881
6.161

3.371
2.521
2.511
2.514
2.510

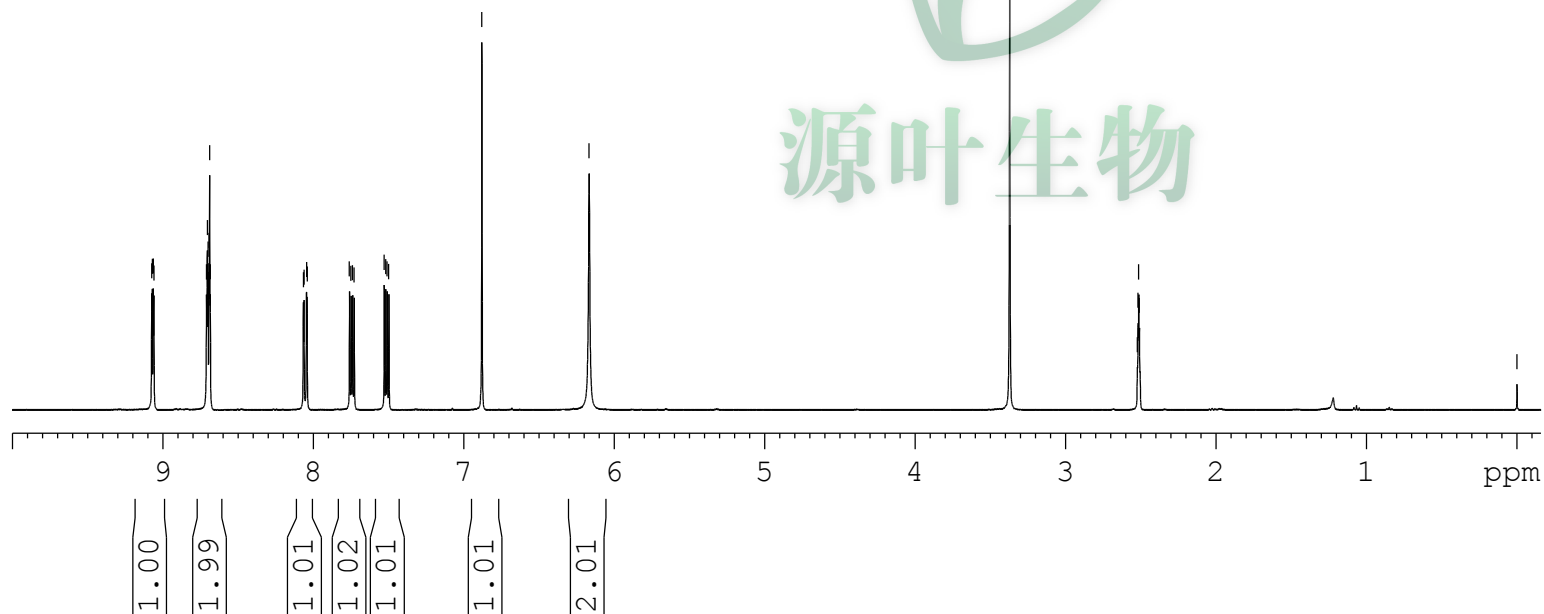

NAME S48167
EXPNO 400
PROCNO 1
Date_ 20191209
Time_ 18.06
INSTRUM spect
PROBHD 5 mm dual

PULPROG zg30
TD 65536
SOLVENT DMSO
NS 8
DS 0
SWH 8620.689 Hz
FIDRES 0.131541 Hz
AQ 3.8011379 sec
RG 203
DW 58.000 usec
DE 6.50 usec
TE 300.0 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
NUC1 1H
P1 13.22 usec
PL1 -3.00 dB
PL1W 20.99974442 W
SFO1 400.1319006 MHz
SI 32768
SF 400.1300012 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00