


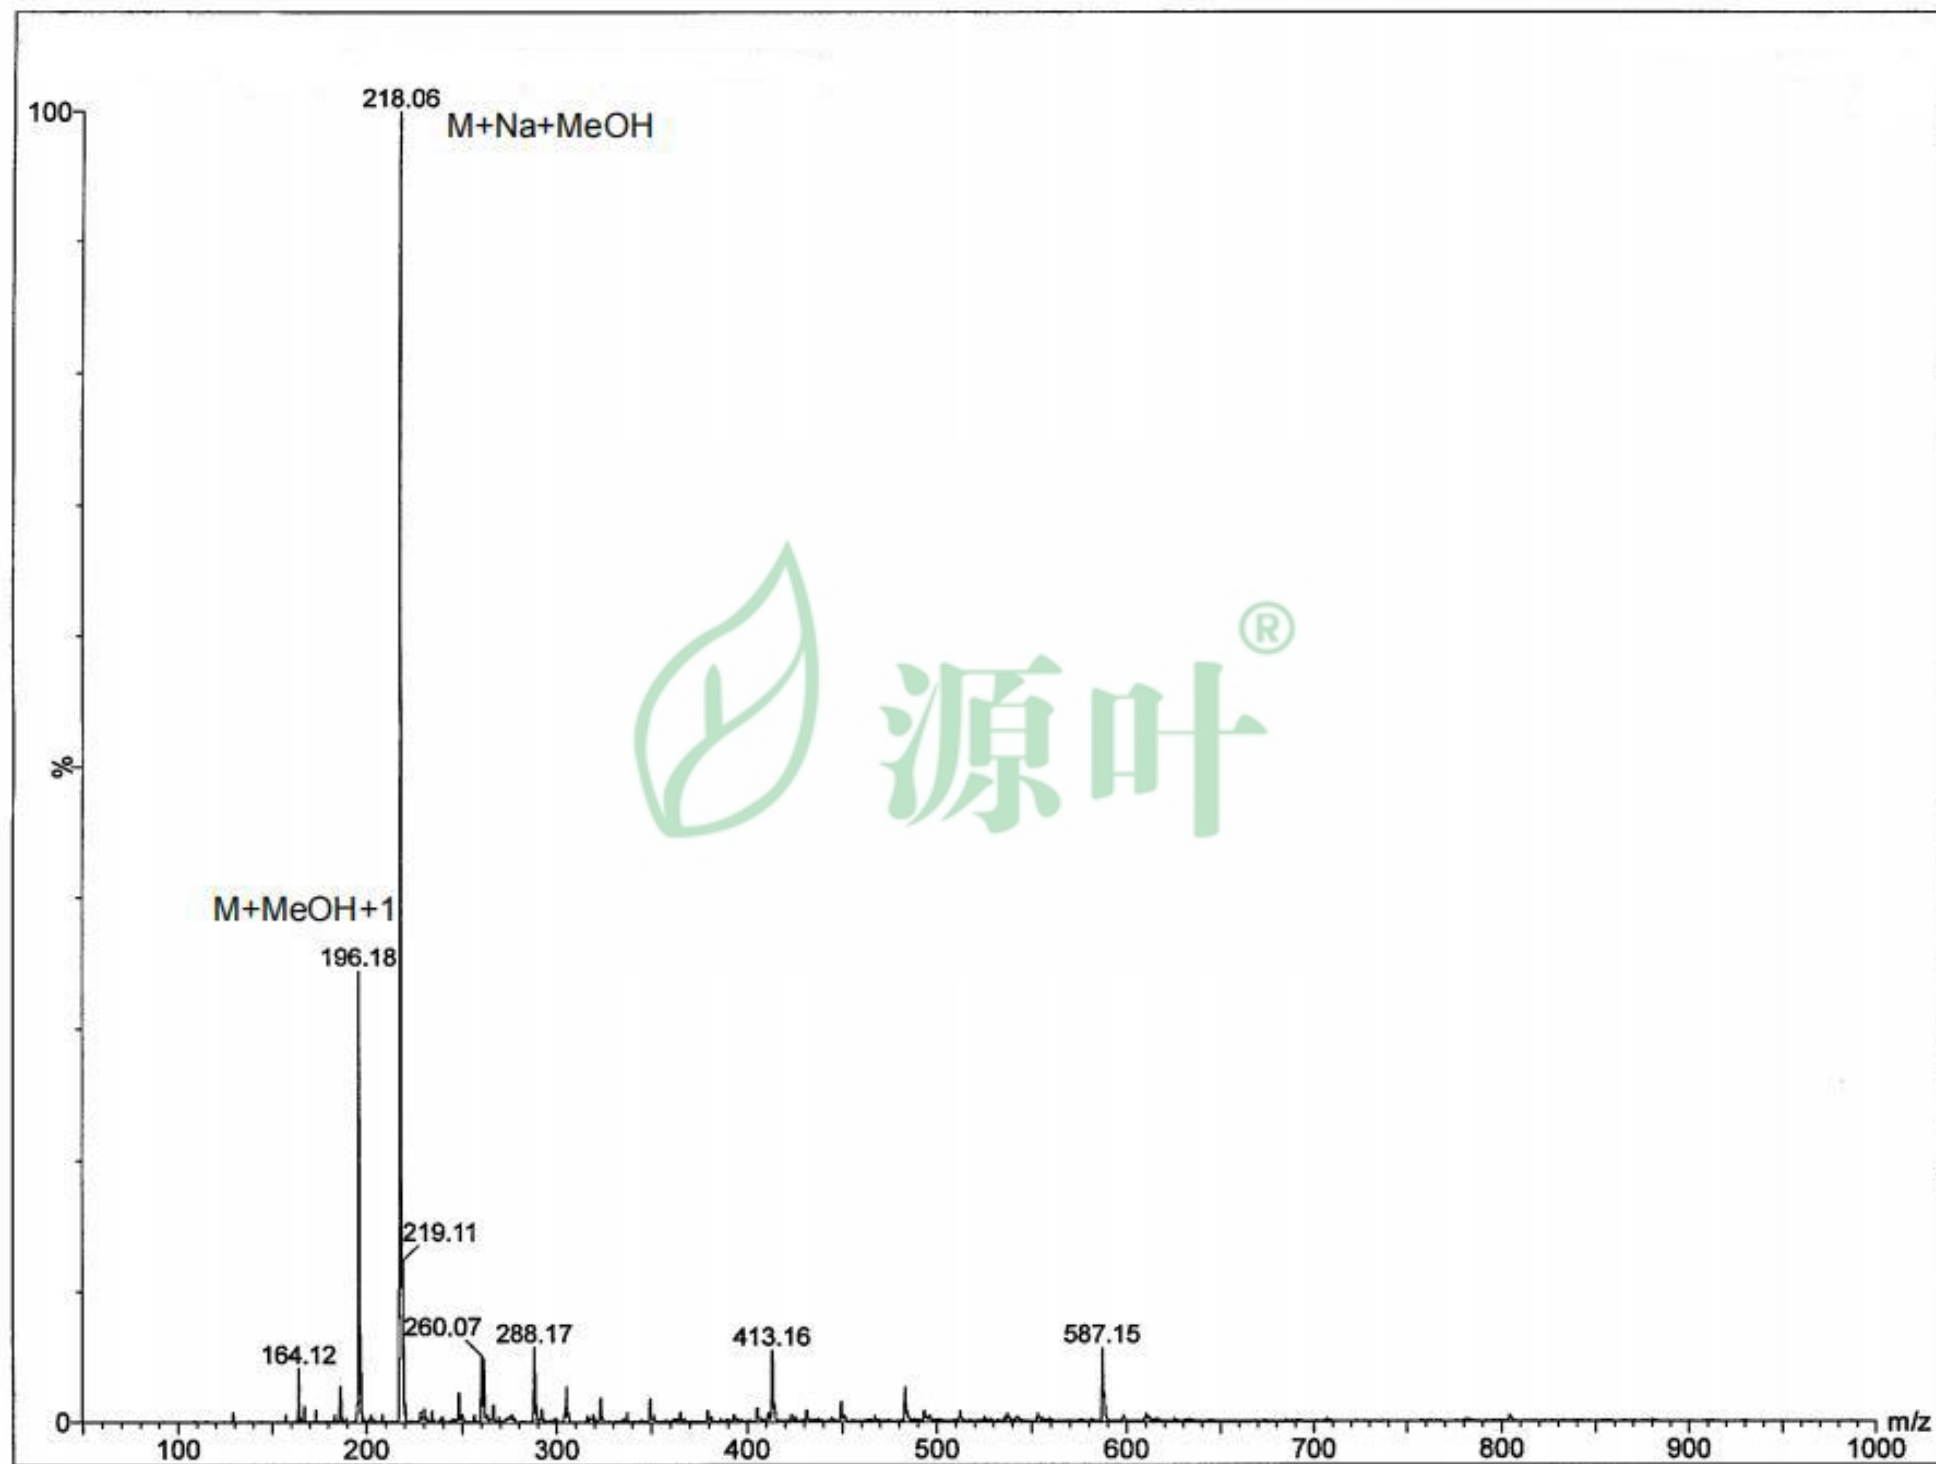
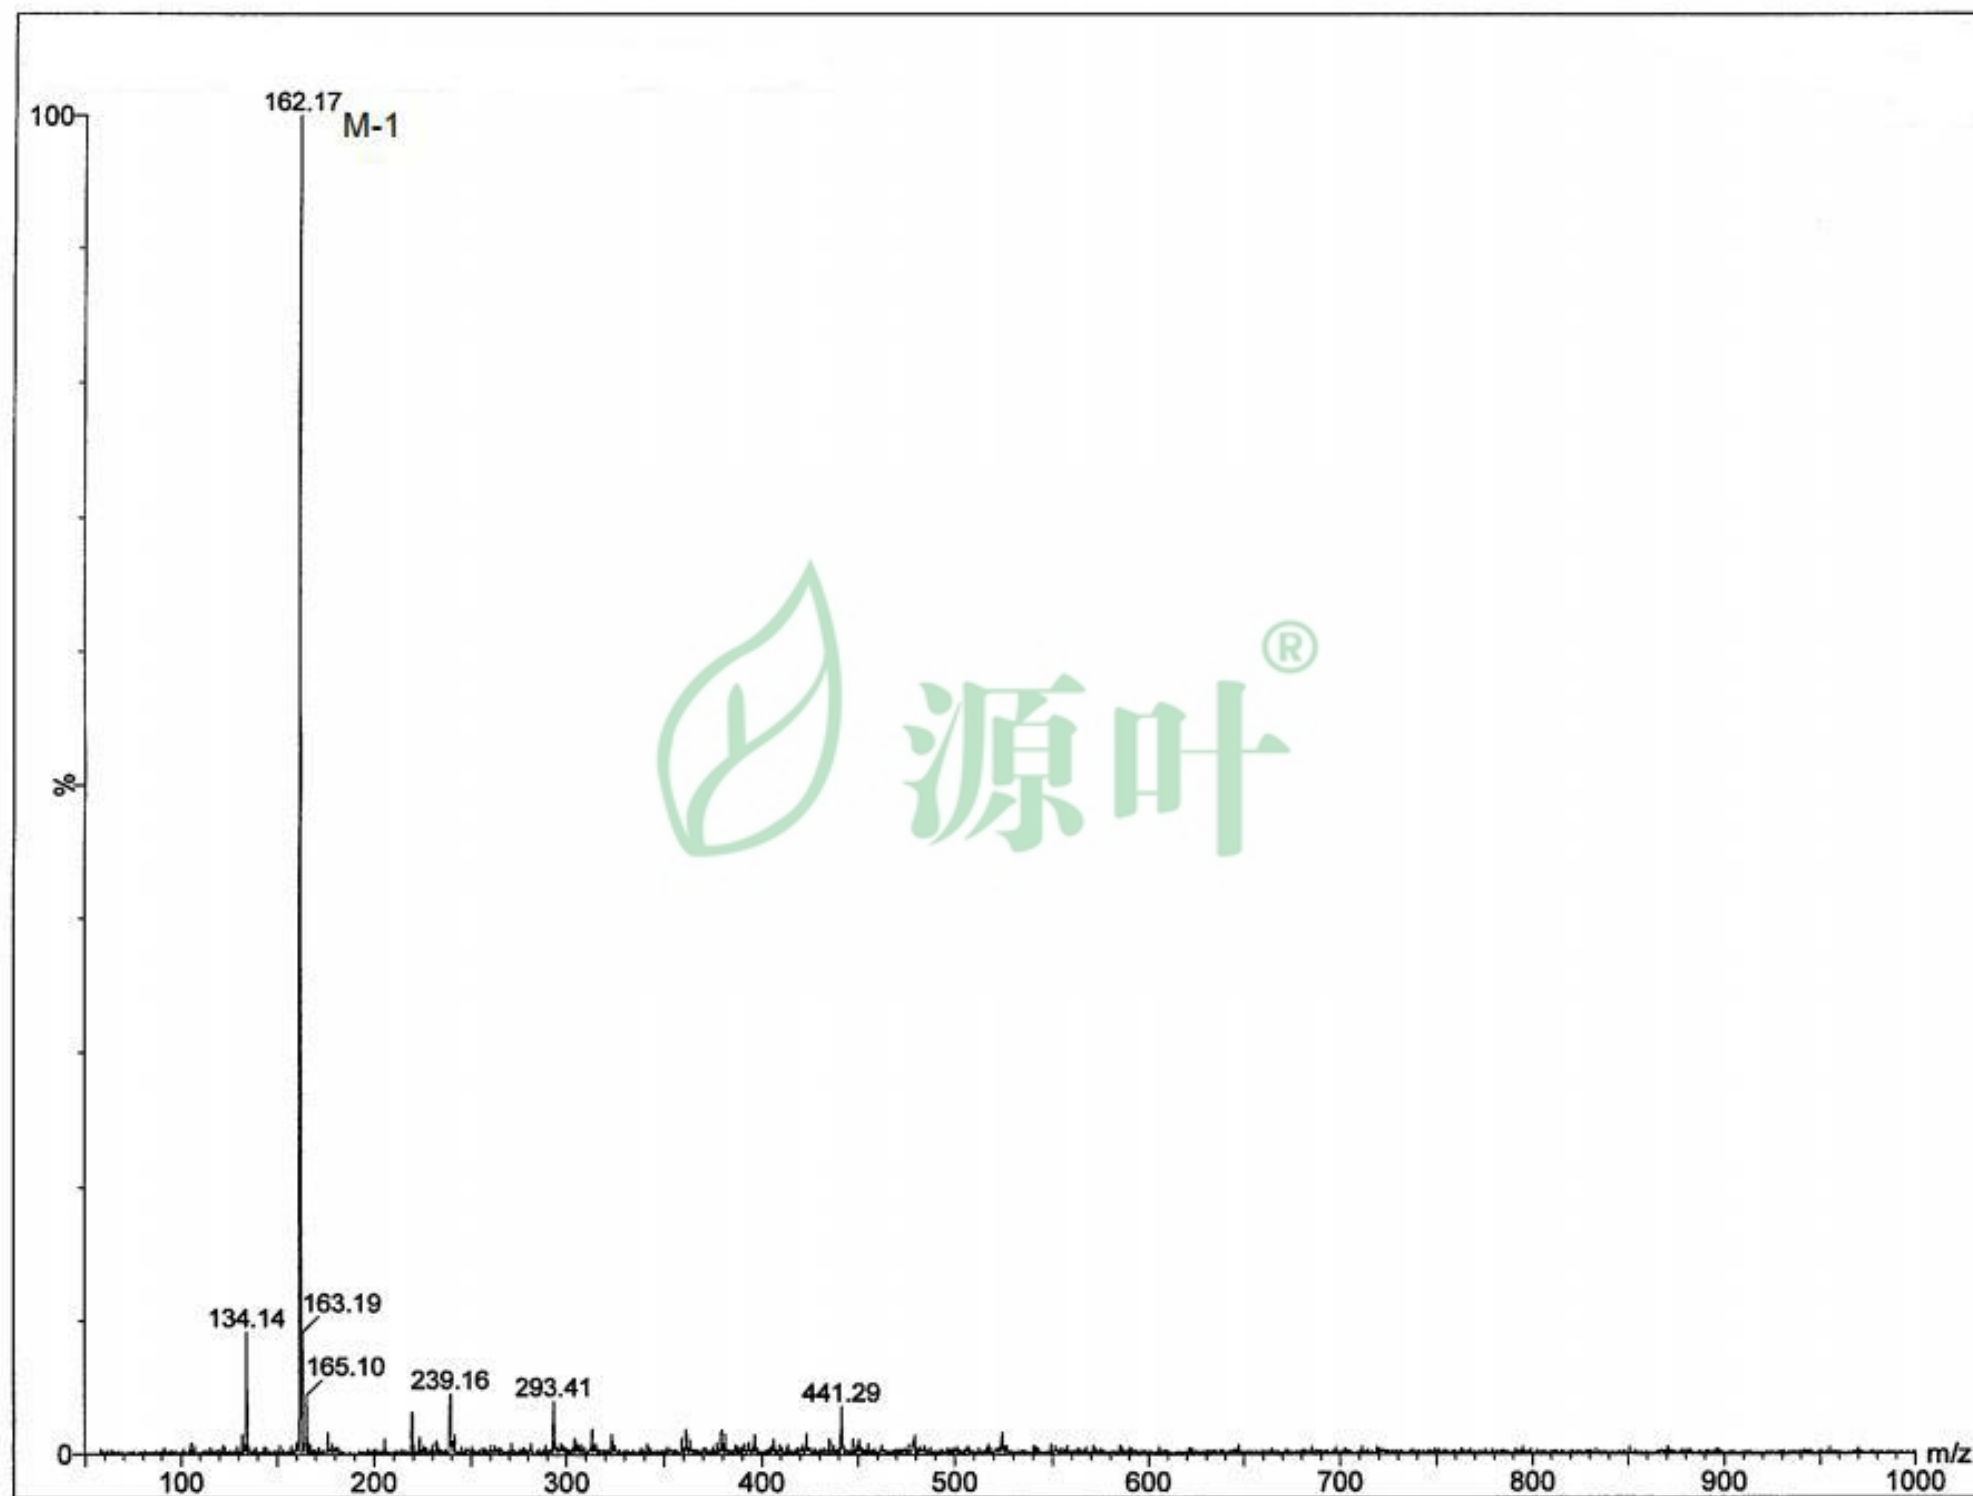


163.06







Current Data Parameters
NAME 2-PEQ-159-1, 19Mar2021u
EXPNO 18
PROCNO 1

F2 - Acquisition Parameters
Date_ 20210319
Time 11.08 h
INSTRUM spect
PROBHD X104450_0350 (
PULPROG zg30
TD 32768
SOLVENT CDCl3
NS 8
DS 1
SWH 7211.539 Hz
FIDRES 0.440157 Hz
AQ 2.2719147 sec
RG 203
DW 69.333 usec
DE 6.50 usec
TE 300.4 K
D1 1.00000000 sec
TDO 1
SFO1 400.1528010 MHz
NUC1 1H
PC 4.43 usec
P1 13.30 usec
PLW1 14.30900002 W

F2 - Processing parameters
SI 32768
SF 400.1500000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 10.00

