


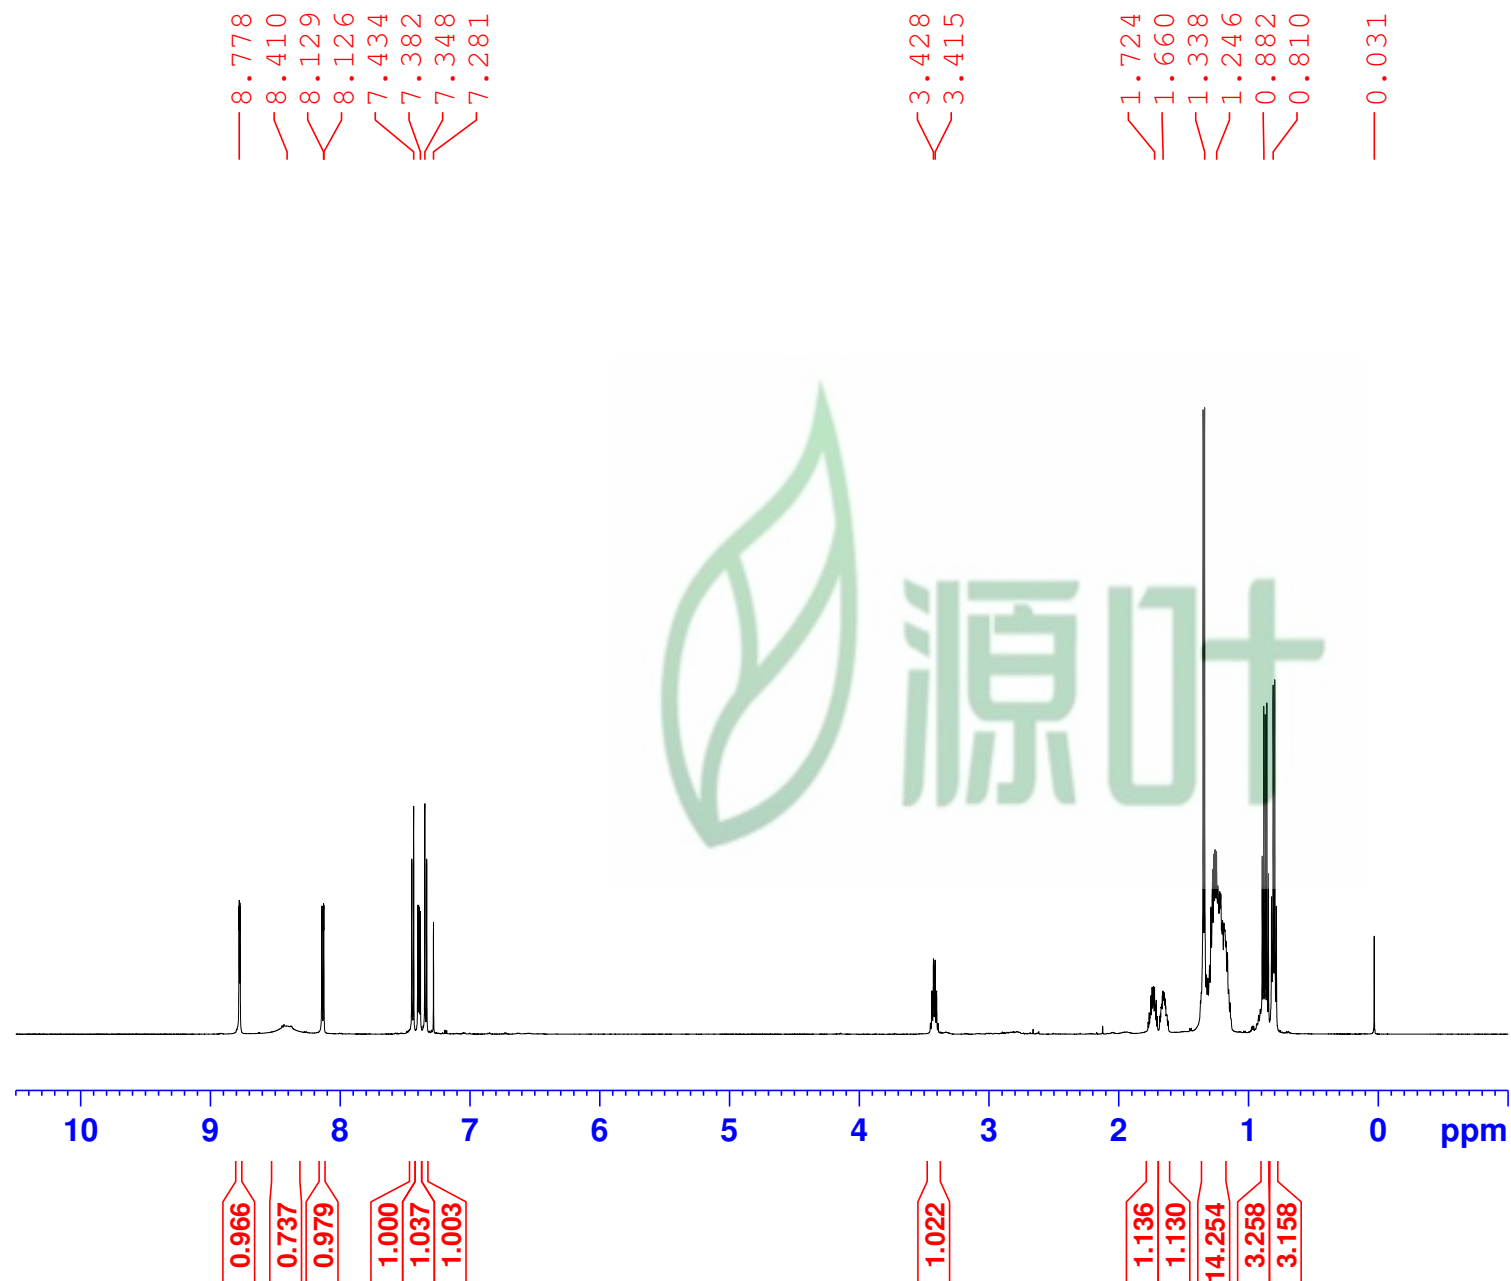

Current Data Parameters
NAME 73545-11-6
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 19.56 h
Time 19.56 h
INSTRUM Avance
PROBHD Z154705_0134 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 0
SWH 11904.762 Hz
FIDRES 0.363304 Hz
AQ 2.7525120 sec
RG 36
DW 42.000 usec
DE 8.79 usec
TE 297.7 K
D1 1.00000000 sec
TD0 1
SFO1 600.1537059 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
PLW1 21.87999916 W

F2 - Processing parameters
SI 65536
SF 600.1500019 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00